

Name: little 2, bird

OS



ID: 0000

Exam Date: 26/07/2021

CZMI

DOB: 1/07/2020

Exam Time: 5:09 PM

Gender: Unknown


Serial Number: 5000-5626

Technician: Operator, Cirrus



Signal Strength: N/A

Anterior Chamber Analysis : Anterior Chamber

OD ☐ ☒ OS

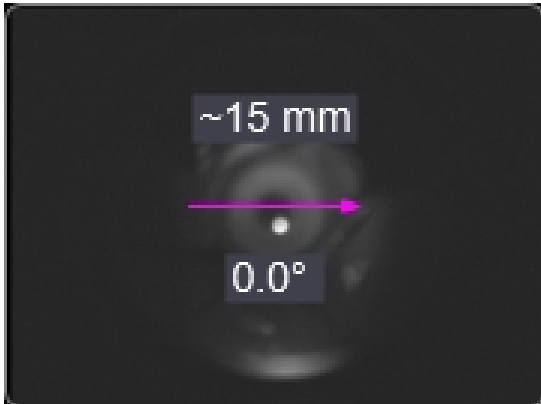

Chamber Measurement	Value
Area	16.35 mm ²

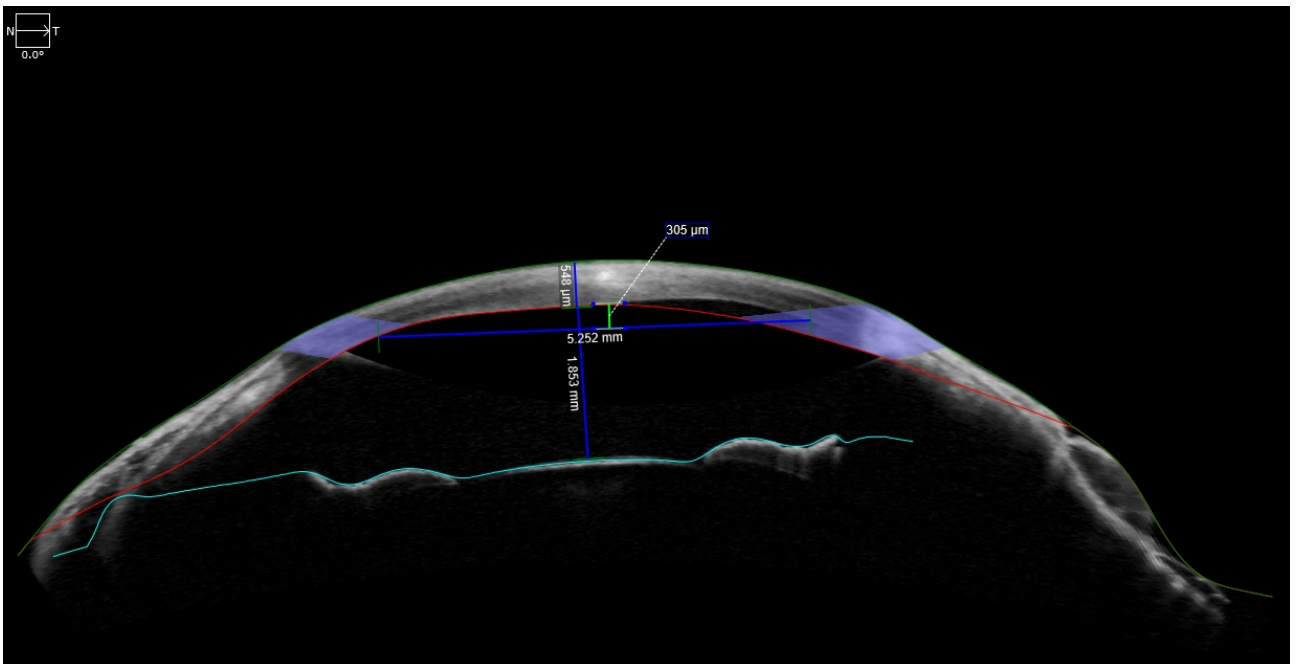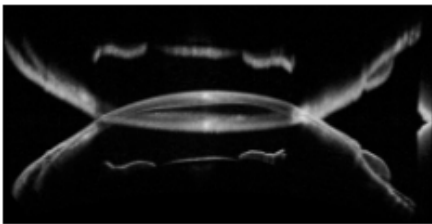

Comments

Doctor's Signature

SW Ver: 11.5.2.54532
Copyright 2020
Carl Zeiss Meditec, Inc
All Rights Reserved

Analysis Edited: 13/10/2021 5:15 PM

Page 1 of 1